

Original article:

**AMPHETAMINES ANALYSIS IN WASTEWATERS -
METHOD PERFORMANCE OF SOLID PHASE EXTRACTION -
HIGHER PERFORMANCE LIQUID CHROMATOGRAPHY MASS
SPECTROMETRY TECHNIQUES (SPE-HPLC MS/MS)**

Aliru Olajide Mustapha^{1*}, Usman L Ajao²

¹ School of Science and Technology, Erasmus Darwin Building ERD 200, Nottingham Trent University, Clifton Lane, NG11 8NS, UK

² Department of Chemistry, University of Ilorin, P.M.B. 1515, Ilorin, Kwara State, Nigeria

* Corresponding author: ammbarsaliu@yahoo.com

ABSTRACT

Recently, many articles have reported different levels and distribution of amphetamine hitherto detected in biological fluids now appreciably found in aquatic environment at ng/L levels. Identification and measurement of amphetamine and its metabolites in surface and sewage waters using higher performance liquid chromatographic methodologies in the literatures now on current trend have provided information that are of scientific interest and effectively replaced immunological methods which only suggest the presence of these substances. Active research on both distribution and impacts of this important drug of abuse and related metabolites in the wastewaters are on-going.

Keywords: amphetamine, solid phase extraction, wastewaters, higher performance chromatography, drug metabolites

INTRODUCTION

The survey of reported liquid chromatography tandem mass spectrometry (HPLC-MS/MS) methods from literatures for the determination of amphetamine and human metabolites in waters (van Nuijs et al. 2009a; Zuccato et al., 2005, 2008; Castiglioni et al., 2006; Hearn et al., 1991; Bones et al., 2007) is discussed in this paper. The higher performance liquid chromatography-mass spectrometry (HPLC-MS) or with tandem mass spectrometry (HPLC-MS/MS) were becoming popular in their separation and detection capabilities, as they appear very rapid, sensitive and selective method at ng/mL concentration levels. The concentrations of amphetamine and its metabolites in aqueous media using HPLC-MS or HPLC-MS/MS appeared to have largely replaced GC-MS in the analysis of

illicit substances particularly in aqueous media. The extraction volumes, mobile phases, detectors (interfaces) and acquisition modes used by different scientists to provide sensitivity and selectivity are shown. The separation procedures rely on the principles of reversed-phase columns with different solvent gradients depending on applications. Tabulated are limits of quantifications depending on matrices for quantification and confirmation of drugs. Recently, variations over convectional HPLC-MS method have appeared in the literature with the name: Ultra-performance liquid chromatography (UPLC-MS/MS) is unique for its short columns packed with small particles sizes and stability at pH range (Bijlsma et al., 2009; Wood et al., 2005; Huerta-Fontela et al., 2008a; Boleda et al., 2007; Kasprzyk-Hordern et al., 2007, 2008). With the development of this rela-

tively new technology, a shorter analysis times as well as gain in separation, efficiency, resolution and sensitivity have been reported. To minimize the effects of ion suppression on the analytical signal, a relatively new HILIC (Hydrophilic interaction chromatography) technique was also carried out in some experiments. Since analytes were better retained on HILIC column, unaffected by ion suppression and a reduction in analytical signal was minimised, the possibilities of using HILIC approach in the quantitative determination of polar compounds such as amphetamine and its metabolites was apparently justified (van Nuijs et al., 2009b; Gheorghe et al., 2008). The use of MS/MS with triple quadrupole (QqQ) analyzers with electrospray ionization (ESI⁺) were mostly used in selected reaction monitoring mode (SRM) to minimize the matrix interferences. The choices of ionization in ESI positive-ion mode were to have achieved ionizations and simultaneous determinations of analytes.

To assess inherent selectivity and peculiar reservations of each method based on the compound and its metabolites wide range of polarities and extraction challenges from different aquatic (wastewater, sediment, sludge) matrices, this paper therefore hopes to review the high quality work published in the literature on amphetamine and its metabolites using HPLC methods to maximise future application needs.

AMPHETAMINE AND METABOLITES

Among the drugs classified as amphetamines are amphetamines (AM), methamphetamines (MA, “speed”) and methylenedioxyamphetamine (MDMA, “ecstasy or Adam”). They are usually taken orally but can be snorted, smoked or injected. They are addictive stimulant drugs that affect the central nervous system among other risks of dependence and abuse. Other designer drugs are methylenedioxyamphetamine (MDE, “eve”) and 3,4-methylenedioxyamphetamine (MDA, “love pills”) (EMCDDA, 2007).

The major metabolic pathway involves deamination of cytochrome P450 to para-hydroxyl amphetamine and phenylacetone, this later compound is oxidised to benzoic acid and excreted as glucuronide or glycine (hippuric acid) conjugates. Smaller amounts of amphetamine are also converted to norephedrine by oxidation. Although most enzymes involved in amphetamine metabolism have not been clearly defined, CYP2D6 is known to be involved with the formation of 4-hydroxyamphetamine.

Since CYP2D6 is genetically polymorphic, population variation in amphetamine metabolism are a possibility (Ensslin et al., 1996). Figure 1 shows that MDMA generates free and conjugated MDA, which is a common metabolite of MDE and MDMA. Other metabolites from MDMA are 4-hydroxy-3-methoxymethamphetamine, HMMA and 4-hydroxy-3-methoxyamphetamine, HMA (Kloss et al., 1984). With normal urine pHs, approximately half of an administered dose of amphetamine is excreted as derivatives of alpha-hydroxyamphetamine and another approximately 30-40 % of the dose can be excreted as parent amphetamine, this is because the urinary recovery of amphetamine is depending on pH and urine flow rate (Dollery, 1991).

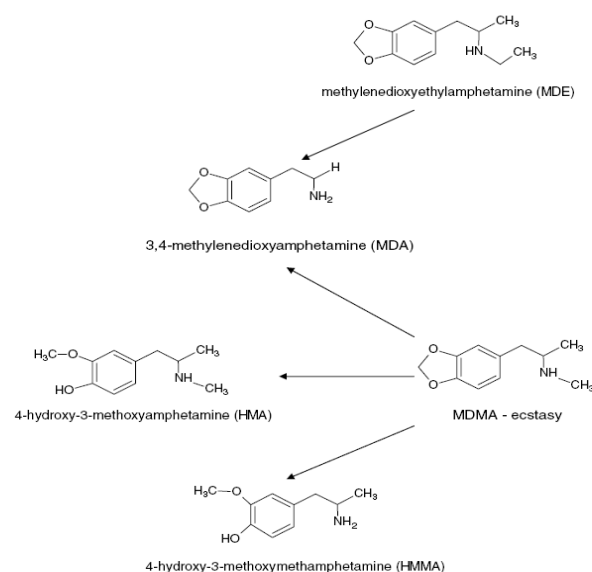


Figure 1: Main metabolites of 3,4-methylenedioxyamphetamine (MDMA) in urine (Kloss et al., 1984)

HPLC-MS/MS METHODOLOGIES

Emerging contaminants of various biological active compounds, pharmaceuticals, personal care products, herbicides and antibiotics are present in complex and varying compositions in wastewaters and sewages. The procedures employed by different authors and published in the literatures in the past decade which include sample pre-concentration as an important step to the determination of amphetamine and related metabolites, followed by higher performance liquid chromatographic-tandem mass spectrometry separation and detection have been reviewed and summarised in Table 1 (at the end of this paper).

Sample pre-concentration

Improved sample clean-ups, pre-treatment, chromatographic separation, centrifugation, filtration, alternative ionization and the use of deuterated compounds as surrogate standards have been employed by authors (Kloss et al., 1984; van Viet et al., 1990; Ellenhorn and Barceloux 1988; Kolbrich et al., 2006; Cone, 1995; Hilton and Thomas, 2003; Marais and Laurens, 2009) to reduce the signal effects thereby correcting the matrix influences. To avoid sample degradation, dark-glass bottles with samples stored at -20 °C at a pH of 6 have been recommended (Hearn et al., 1991; Bones et al., 2007; Bijlsma et al., 2009; Wood et al., 2005). Solid phase extraction using different extraction protocols achieving different extraction method recoveries of 50-105 %, (Kloss et al., 1984); 50-65 % (Ellenhorn and Barceloux, 1988); 73-96 % (Hummel et al., 2006); 90 % (Hilton and Thomas, 2003), and 65-106 % (Drummer et al., 2007) respectively. When using HPLC-MS/MS with electro spray ionization detector (ESI) as interface, the matrix effect is one of the major factors affecting the isolation and analysis of drugs in complex matrices like wastewaters and sewages (Hummel et al., 2006).

mel et al., 2006). Co-elution of matrix substituents causes suppression or enhancement of signal which ultimately affects the accuracy and reliability of results.

Amphetamine in the aqueous environment

The major metabolites that have been so found and quantified are summarised in Table 2. However, the presence of some human amphetamine metabolites identified in biological fluids (Kloss et al., 1984; Cone, 1995; Ambre, 1985; Chen et al., 2008; Zhang and Zhou, 2007; Quintana et al. 2005; Wylie et al., 2005; Yu et al., 2009) are yet to reported in the aquatic environment.

Table 2: Amphetamine and metabolites

Human metabolites identified in biological fluids	Human metabolites identified in the aquatic environment
<i>Chen et al., 2008;</i> <i>Zhang and Zhou, 2007;</i> <i>Quintana et al., 2005;</i> <i>Wylie et al., 2005;</i> <i>Yu et al., 2009</i>	<i>Kloss et al., 1984;</i> <i>Ellenhorn and Barceloux, 1988;</i> <i>Cone, 1995;</i> <i>Ambre, 1985</i>
Amphetamine	detected
Metamphetamine	detected
<i>p</i> -OHMA	not detected
<i>p</i> -OHMA-Glu	not detected
<i>p</i> -OHMA-Sul	not detected
MDA	detected
MDMA	detected
MDEA	detected
MBDB	detected

In many parts of Europe, amphetamine and its metabolites have been reported in many wastewaters, surface waters and sewage at nanogram and microgram concentration levels with influent samples containing more of amphetamine and metabolites than effluents collected from sewage treatment plants, STPs (Table 3).

Table 3: Amphetamine and metabolites concentration in wastewaters worldwide

Analytes	Matrix	Influent (ng L ⁻¹)	Effluent (ng L ⁻¹)	SW (ng L ⁻¹)	Volume	References
Amphetamines	3 Rivers, Italy Eastern Spain 2 STPs, Italy 42 STPs, NE Spain	- 1400 5.4-14.7 ± 10.6 03-6880	- 110-210 2.8 04-2100	< 0,65 - - -	N/A N/A 1-2 L N/A	Zuccato et al., 2008 Bijlsma et al., 2009 Castiglioni et al., 2006 Huerta-Fontela et al., 2008
	Barcelona, Spain 5 STPs, Spain	20.8-41.1 ± 9.1 15	0.45-2.2 ± 0.1 < 1.0	2.84 < 0.8	1 L 1.5 L	Postigo et al., 2008 Huerta-Fontela et al., 2008
Metamphet-amine	5 STPs, Nebraska, USA	1.3 ± 0.1-1.4	3501 ± 78.3	-	2.5 L	Bartelt-Hunt et al., 2009
	Eastern Spain 2 STPs, Italy 42 STPs, NE Spain	- < 500 3-277	< 100-540 < 1.11-3.5 ± 2 3-90	- - -	N/A 1-2 L N/A	Bijlsma et al., 2009 Castiglioni et al., 2006 Huerta-Fontela et al., 2008
	3 STPs, USA	15 ± 2-66 ± 14	0.8-1.3	-	N/A	Jones-Lepp et al., 2004
	Barcelona, Spain Murray, USA	4.8-18.2 ± 5.8 6.0-34	2.1-6.3 ± 0.6 03-7	2.87 -	1 L 2 L	Postigo et al., 2008 Hearn et al., 1991
MDA	42 STPs, NE Spain	03-266	01-200	-	N/A	Huerta-Fontela et al., 2008
	3 Rivers, Italy Eastern Spain 2 STPs, Italy 5 STPs, Spain	- 500-1400 4.6 ± 7.3-8.7 03-266	- 410-680 0.9 ± 1.9-1.1 ± 1.5 1-200	3 ± 0.3-4 - - -	N/A N/A 1-2 L 1.5 L	Zuccato et al., 2005 Bijlsma et al., 2009 Castiglioni et al. 2006 Huerta-Fontela et al., 2008
MDMA	3 Rivers, Italy Eastern Spain 2 STPs, Italy 5 STPs, Spain	- 326-2700.5 13.6 ± 12.6-14.2 ± 14.5 91	- 100-2100.2 4.4 ± 3.7-5.1 ± 3 67	1.1-4.0 - - 3.5	N/A N/A N/A 1.5 L	Zuccato et al., 2008 Bijlsma et al., 2009 Castiglioni et al., 2006 Huerta-Fontela et al., 2008
	STP, Italy	2-598	2-267	-	1 L	Huerta-Fontela et al., 2008
	Barcelona, Spain Murray, USA 42 STPs, NE Spain	133-135.13 ± 29.8 < 1.0-10.0 2-598	82.1-148.2 ± 22.2 - 2-267	129 - -	1 L 2 L N/A	Postigo et al., 2008 Hearn et al., 1991 Huerta-Fontela et al., 2008
	5 STPs, Spain	27	< 2.1	-	1.5 L	Huerta-Fontela et al., 2008
MDEA	2 STPs, Italy STP, Italy STP, Spain	4.19-1.5 ± 3.8 6-114 < 500	< 1.64 12 < 100	- - -	N/A 1 L N/A	Castiglioni et al., 2006 Bijlsma et al., 2009 Huerta-Fontela et al., 2008

HPLC method performances

The survey of reported HPLC-MS/MS methods for the determination of amphetamine and human metabolites in water with the extraction volumes, mobile phases, detectors (interfaces) and acquisition modes used by different scientists to provide sensitivity and selectivity is shown in Table 1.

The application of LC-MS² to the simultaneous analysis of a wide variety of illicit drugs in waste water was first reported by Castiglioni et al. (2006). The HPLC column (XTerra MS C18, 100 x 2.1 mm, 3.5 µm) with four separate total gradient elution times of 28, 32, 36 and 26

min for amphetamines, cocainics, opioids and cannabinoids were reported respectively. Wastewater samples (50 mL) were spiked with 20 ng of internal standards (cocaine-*d*₃, benzoylecgonine-*d*₃, norcocaine-*d*₃, cocaethylene-*d*₈, amphetamine-*d*₆, methamphetamine-*d*₉, MDA-*d*₅, MDMA-*d*₅, MDEA-*d*₅, morphine-*d*₃, morphine-3β-D-glucuronide-*d*₃, 6-acetylmorphine-*d*₆, methadone-*d*₃, EDDP-*d*₃ and 11-nor9-carboxy-Δ-THC-*d*₃) and extracted using a standard Oasis MCX SPE procedure. Quantitation was based on the MH⁺ peak areas of the analyte relative to the MH⁺ peak areas of the corresponding internal standards. The

mobile phase solvent A: acetic acid 0.05 % in water and solvent B: acetonitrile. But solvent A for cannabinoids was triethylamine 0.05 % in water. ESI gave abundant protonated molecule ions (MH^+) for each of the analytes and internal standards. Measured quantitation ranges were: 0.2-1 $\mu\text{g/L}$ for cocaine and its metabolites, 80-200 ng/L for morphine, 10 ng/L for 6-acetylmorphine, 60-90 ng/L for methadone and its metabolite 2-ethylidene-1,5-dimethyl-3,3-diphenylpyrrolidine and lower than 20 ng/L for amphetamines. The overall method variability was $\leq 10\%$ for the influents, $\leq 5\%$ for effluents and recoveries in wastewater were $\geq 80\%$.

The use of Polar Organic Chemical Integrative Samplers (POCIS) methodology for sampling was introduced by Bartelt-Hunt et al. (2009), the samplers were installed in rivers upstream and downstream of treated WWTP at five different sites. The HPLC separation was performed isocratically on a Betabasic-18 column (250 x 2.1 mm, 5 μm , and 50 $^\circ\text{C}$) with a mobile phase of methanol with 0.1 % formic acid in water. The electrospray ionization in positive mode (ESI^+) by multiple reaction monitoring gave the mass spectrum of the analytes. Each of the POCIS devices was removed from its deployment canister, and the contents were transferred with 20 mL high-purity methanol into silane-treated vials, stored at -20 $^\circ\text{C}$ and compounds were eluted with 50 mL of high-purity methanol through silane-treated gas gravity flow chromatography columns into 120 mL evaporation tubes. After addition of the internal standards (metamphetamine- d_9 , $^{13}\text{C}_3$ -caffeine, and $^{13}\text{C}_8$ -sulfamethazine), the eluates were evaporated to approximately 1 mL under nitrogen and quantitatively transferred to autosampler for analysis. The estimated detection limits for most compounds were less than 1 $\text{pg}/\mu\text{L}$ while the averaged recovery was $123 \pm 30\%$; however, the determination of the uptake rates for the compounds of interest for quantitative analysis is the limitation of POCIS.

Ultra-performance liquid chromatography (UPLC-ESI-MS/MS) is a variation

over convectional HPLC-MS method. The ultra-fast LC-MS² is unique for its short columns packed with small particles sizes and stability at pH range; with the development of this relatively new technology, a shorter analysis times as well as gain in separation, efficiency, resolution and sensitivity are introduced (Huerta-Fontela et al., 2008).

The occurrence of psychoactive drugs in wastewaters using the new UPLC-ESI-MS² technique (Huerta-Fontela et al., 2008; Wood et al., 2005) on an Acquity BEH C₁₈ UPLC column, (100mm x 2.1mm i.d., 1.7 μm particle size) after enrichment by solid phase extraction (SPE). The optimized separation conditions were for solvent A: acetonitrile with 0.1 % formic acid; solvent B: 30 mM formic acid/ammonium formate (pH 3.5) at a flow rate of 0.5 mL/min. The ESI working in positive mode with acquisition in selected reaction mode (SRM) gave abundant protonated molecular ion of each compound as the precursor ion: nicotine (163>130; 163>117), cotinine (177>80; 177>98), caffeine (195>138; 195>110), paraxantine (181>124; >181>96), amphetamine (136>119; 136>91), MDA (180>163; 180>105), metamphetamine (150>91; 150>119), MDMA (194>163; 194>105), MDEA (208>163; 208>133), ketamine (238>125; 238>220), cocaine (304>182; 304>105), benzoylecgonine (290>169; 290>150), LSD (324>223; 324>208), PCP (244>85; 244>159) and fentanyl (337>188; 337>105). The LODs were lower than 1.5 ng/L and 300 ng/L where LOQs were lower than 5 ng/L and 850 ng/L , respectively, with the recoveries ranged from 70 to 101 %.

At the University of Glamorgan, Sustainable Environmental Research Centre, UK, Kasprzyk-Hordern et al. (2007) made use of the new, fast and sensitive method for the broad range of pharmaceuticals, illicit drugs which include amphetamines with triple quadrupole tandem mass spectrometry with positive-ion mode (ESI^+) was used for separation of up to 30 compounds on Acquity UPLC BEH C₁₈ column (1.7 μm ; 1 mm x 100mm) with mobile phase A: (pH,

2.8) of 94.5 % of H₂O, 5 % MeOH, 0.5 % CH₃COOH and mobile phase B: (pH, 3.2) of 99.5 % MeOH and 0.5 % CH₃COOH after Oasis MCX, sorbent extraction. The methods limits were of quantification ranged from 0.3 to 50 ng/L with the instrumental limit of quantification from 0.2 to 10 µg/L.

Bijlsma et al. (2009) recently reported use of UPLC-MS/MS method came from for the simultaneous determination of amphetamines, cocaines, cannabis and their metabolites in surface and waste water. After SPE enrichment, the selected drugs were separated on Acquity BEH C₁₈ UPLC column, (50 mm x 2.1 mm i.d., 1.7 µm particle size) with methanol (solvent A) and 5 mM ammonium acetate/0.1 % formic acid (solvent B). The use of MS/MS with triple quadrupole (QqQ) analyzers with electrospray ionization (ESI⁺) was used in selected reaction monitoring mode (SRM) to minimize the matrix interferences. The choice of ionization in ESI positive-ion mode was deliberate to have abundant ionization of THC-COOH as well as simultaneous determinations for all the analytes. The recoveries of 70-120 % were reported with precision of ≤ 20 % for all compounds.

CONCLUSIONS

HPLC-MS has been widely used as a good technique for highly polar, highly molecular weight and thermolabile compounds for the determination of amphetamine and its active metabolites in waters. No hydrolysis, no derivatization, one-step extraction especially with the introduction of API and ESI interfaces, the technique has been popular.

The Oasis MCX was also a good choice because its mixed mode materials during loading, washing and elution steps allows improved selectivity towards basic analytes due to pH and polarity changes. The internal standard was found as valuable tool for standardization and quantification and has almost identical physicochemical properties like the normal drugs and their metabolites analogues. Like cocaine analysis and simi-

lar drugs, the Oasis HLB cartridge built of a hydrophilic and a lipophilic monomer and Oasis MCX cartridge - a mixed reversed-phase/cation-exchange - were common cartridges for drug extraction with good recoveries. However, insufficient reference standards in contrast to GC-MS technique (which has large data bases of mass spectral) has made HPLC less attractive in studies where structural confirmation is needed.

REFERENCES

Ambre J. The urinary excretion of cocaine and metabolites in humans: a kinetic analysis of published data. *Journal of analytical toxicology* 1985;9:241-5.

Bartelt-Hunt SL, Snow DD, Damon T, Shockley J, Hoagland K. The occurrence of illicit and therapeutic pharmaceuticals in wastewater effluent and surface waters in Nebraska. *Environ Pollut* 2009;157:786-91.

Bijlsma L, Sancho JV, Pitarch E, Ibanez M, Hernandez F. Simultaneous ultra-high-pressure liquid chromatography-tandem mass spectrometry determination of amphetamine and amphetamine-like stimulants, cocaine and its metabolites, and a cannabis metabolite in surface water and urban wastewater. *J Chromatogr* 2009;A1216:3078-89.

Boleda MR, Galceran MT, Ventura F. Trace determination of cannabinoids and opiates in wastewater and surface waters by ultra-performance liquid chromatography-tandem mass spectrometry. *J Chromatogr* 2007;A1175:38-48.

Bones J, Thomas KV, Paull B. Using environmental analytical data to estimate levels of community consumption of illicit drugs and abused pharmaceuticals. *J Environ Monit* 2007;9:701-7.

- Castiglioni S, Zuccato E, Crisci E, Chiabrando C, Fanelli R, Bagnati R. Identification and measurement of illicit drugs and their metabolites in urban wastewater by liquid chromatography-tandem mass spectrometry. *Anal Chem* 2006;78: 8421-9.
- Chen HC, Wang PL, Ding WH. Using liquid chromatography-ion trap mass spectrometry to determine pharmaceutical residues in Taiwanese rivers and wastewater. *Chemosphere* 2008;72:863-9.
- Cone EJ. Pharmacokinetics and pharmacodynamics of cocaine. *J Anal Toxicol* 1995;19:459-78.
- Dollery CT. Clinical pharmacology of calcium antagonists. *Am J Hypertension* 1991;4:88S-95S.
- Drummer OH, Gerostamoulos D, Chu M, Swann P, Boorman M, Cairns I. Drugs in oral fluid in randomly selected drivers. *Forensic Sci Int* 2007;170:105-10.
- Ellenhorn MJ, Barceloux DG. Medical toxicology: diagnosis and treatment of human poisoning. New York: Elsevier, 1988 (pp 644-661).
- Ensslin HK, Kovar K, Maurer HH. Toxicological detection of the designer drug 3,4-methylenedioxyethylamphetamine (MDE, "Eve") and its metabolites in urine by gas chromatography - mass spectrometry and fluorescence polarization immunoassay. *J Chromatogr* 1996;B683:189-97.
- EMCDDA, European Monitoring Centre for Drugs and Drug Addiction. The state of the drug problem in the European Union and Norway. Annual report 2007. Lisbon, Portugal. Available from: [http://www.emcdda.europa.eu/attachments.4m/att-42156-EN-TDA \(07001ENG.pdf\)](http://www.emcdda.europa.eu/attachments.4m/att-42156-EN-TDA (07001ENG.pdf)).
- Gheorghe A, van Nuijs A, Pecceu B, Bervoets L, Jorens PG, Blust R et al. Analysis of cocaine and its principal metabolites in waste and surface water using solid-phase extraction and liquid chromatography-ion trap tandem mass spectrometry. *Anal Bioanal Chem* 2008;391:1309-19.
- Hearn WL, Flynn DD, Hime GW, Rose S, Cofino JC, Mantero-Atienza E et al. Cocaine ethylene: a unique cocaine metabolite displays high affinity for the dopamine transporter. *J Neurochem* 1991;56:698-701.
- Hilton MJ, Thomas KV. Determination of selected human pharmaceutical compounds in effluent and surface water samples by high-performance liquid chromatography-electrospray tandem mass spectrometry. *J Chromatogr* 2003;A1015:129-41.
- Huerta-Fontela M, Galceran MT, Martin-Alonso J, Ventura F. Occurrence of psychoactive stimulatory drugs in wastewaters in north-eastern Spain. *Sci Total Environ* 2008;397:31-40.
- Hummel D, Löffler D, Fink G, Ternes TA. Simultaneous determination of psychoactive drugs and their metabolites in aqueous matrices by liquid chromatography mass spectrometry. *Environ Sci Technol* 2006;40:7321-8.
- Jones-Lepp TL, Alvarez DA, Pelly JD, Huckins JN. Polar organic chemical integrative sampling and liquid chromatography-electrospray/Ion-Trap-Mass Spectrometry for assessing selected prescription and illicit drugs in treated sewage. *Arch Environ Contam Toxicity* 2004;47:427-39.
- Kasprzyk-Hordern B, Dinsdale RM, Guwy AJ. Multi-residue method for the determination of basic/neutral pharmaceuticals and illicit drugs in surface water by solid-phase extraction and ultra-performance liquid chromatography-positive electrospray ionization tandem mass spectrometry. *J Chromatogr* 2007;A1161:132-45.

- Kasprzyk-Hordern B, Dinsdale R, Guwy AJ. The occurrence of pharmaceuticals, personal care products, endocrine disruptors and illicit drugs in surface water in South Wales, UK. *Water Res* 2008;42:3498-518.
- Kloss MW, Rosen GM, Rauckman EJ. Bio-transformation of norcocaine to norcocaine nitroxide by rat brain microsomes. *Psychopharmacology* 1984;84:221-4.
- Kolbrich EA, Barnes AJ, Gorelick DA, Boyd SJ, Cone EJ, Huestis MA. Major and minor metabolites of cocaine in human plasma following controlled subcutaneous cocaine administration. *J Anal Toxicol* 2006;30:501-10.
- Marais AAS, Laurens JB. Rapid GC–MS confirmation of amphetamines in urine by extractive acylation. *Forensic Sci Int* 2009;183:78-86.
- Postigo C, de Alda MJ, Barcelo D. Fully automated determination in the low nanogram per litre level of different classes of drugs of abuse in sewage water by on-line solid-phase extraction-liquid chromatography-electrospray-tandem mass spectrometry. *Anal Chem* 2008;80:3123-34.
- Quintana JB, Weiss S, Reemtsma T. Pathways and metabolites of microbial degradation of selected acidic pharmaceutical and their occurrence in municipal wastewater treated by a membrane bioreactor. *Water Res* 2005;39:2654-64.
- van Nuijs ALN, Pecceu B, Theunis L, Dubois N, Charlier C, Jorens PG et al. Spatial and temporal variations in the occurrence of cocaine and benzoylecgonine in waste- and surface water from Belgium and removal during wastewater treatment. *Water Res* 2009a;43:1341-9.
- van Nuijs ALN, Pecceu B, Theunis L, Dubois N, Charlier C, Jorens PG et al. Cocaine and metabolites in waste and surface water across Belgium. *Environ Poll* 2009b;157:123-9.
- van Viet H, Chevalier P, Sereni C, Bornet P, Bautier P, Degos CF et al. Neurologic complications of cocaine abuse. *Presse Méd* 1990;19:1045-9.
- Wood M, Laloup M, Fernandez MDMR, Jenkins KM, Young MS, Ramaekers JG et al. Quantitative analysis of multiple illicit drugs in preserved oral fluid by solid-phase extraction and liquid chromatography–tandem mass spectrometry. *Forensic Sci Int* 2005;150:227-38.
- Wylie FM, Torrance H, Anderson RA, Oliver JS. Drugs in oral fluid: Part I. Validation of an analytical procedure for licit and illicit drugs in oral fluid. *Forensic Sci Int* 2005;150:191-8.
- Yu L, Fink G, Wintgens T, Melin T, Ternes TA. Sorption behavior of potential organic wastewater indicators with soils. *Water Res* 2009;43:951-60.
- Zhang ZL, Zhou JL. Simultaneous determination of various pharmaceutical compounds in water by solid-phase extraction–liquid chromatography–tandem mass spectrometry. *J Chromatogr* 2007;A1154:205-13.
- Zuccato E, Chiabrando C, Castiglioni S, Calamari D, Bagnati R, Schiarea S et al. Cocaine in surface waters: a new evidence-based tool to monitor community drug abuse. *Environ Health: a global access science source* 2005;4:14.
- Zuccato E, Castiglioni S, Bagnati R, Chiabrando C, Grassi P, Fanelli R. Illicit drugs, a novel group of environmental contaminants. *Water Res* 2008;42:961-8.

Table 1: Survey of reported HPLC-MS/MS methods for the determination of amphetamine and human metabolites in water (2000-2010)

Analytes	Matrix	Sample preparation			LC		MS		Method LOQ (ng/L)	Reference
		Volume (mL)	Extraction	Method Recovery (%)	Chromatographic column	Mobile phase	Detector (interface)	Acq. mode		
1 ALC	WW	500 mL	SPE (Strata-XC, 200 mg)	50-65 %	HPLC: Phenomenex Onyx C ₁₈ (200 x 3.0 mm i.d.)	NR	NR	NR	36-120	Bones et al., 2007
5 ALCs	WW	50 mL	SPE (Oasis, MCX, 60 mg)	50-105 %	HPLC: XterraMS C ₁₈ (100 mm x 2.1 mm, 3.5 µm)	250 µL/min A: CH ₃ COOH/ H ₂ O B ₁ : AcN A ₂ 0.05 % TEA/H ₂ O	QqQ (EST ⁺)	MRM	300 pg/L ^{wwinf} 1 ng/L ^{wweff}	Castiglioni et al., 2006
1 ALC	WW	250 mL	SPE (Oasis, HLB, 200 mg)	36-49 %	HPLC: Varian Pursuit XR _s C ₁₈ (100 mm x 2.0 mm, 3 µm)	A: de-ionized water/ 0.5 % HCOOH B: 82 % CH ₃ OH/ 18 %/AcN/ 0.5 % HCOOH		Scan (CID)	0.25-5.0	Hearn et al., 1991
5 ALCs	WW	100 mL	SPE (Oasis, HLB, 200 mg)	70-110 %	UPLC: Acquity BEH C ₁₈ (100 mm x 2.1 mm, 1.7 µm)	A: AcN/0.1 % HCOOH B: 30 mM HCOOH/NH ₄ HCO ₂ (pH 3.5)		QqQ (EST ⁺)	5 and 850	Huerta-Fontela et al., 2008
1 ALC	SW	100 mL	SPE (Oasis, MCX, 60 mg)	65-106 %	UPLC: Acquity BEH C ₁₈ (1.7 µm, 1 mm x 100 mm)	A: 94.5 % H ₂ O 5 % MeOH, 5 % CH ₃ COOH (pH 2.8) B: 99.5 % MeOH + 0.5 % CH ₃ COOH (pH 3.2)	QqQ (EST ⁺)	MRM	0.3-50	Kasprzyk-Hordern et al. 2007

Acq. mode - Acquisition mode- SRM, Selected reaction monitoring; CID, Collision-induced dissociation. Detector and interface used – QqQ, Triple quadrupole; ITMS, Ion Trap mass spectrometry, ESI, Electrospray ionization. MeOH – Methanol; TEA, Triethylamine; NH₄HCO₂, Ammonium acetate; AcN, Acetonitrile, H₂O, Water. WW, Wastewater; SW, Surface water; WW^{inf}, Waste water influent; WW^{eff}, Waste water effluent. RPLC, Reversed-phase liquid chromatography; UPLC, Ultra-performance liquid chromatography; HILIC, Hydrophilic interaction chromatography. ALCs: amphetamine-like compounds